


Roche in Haemostasis

Bibliography



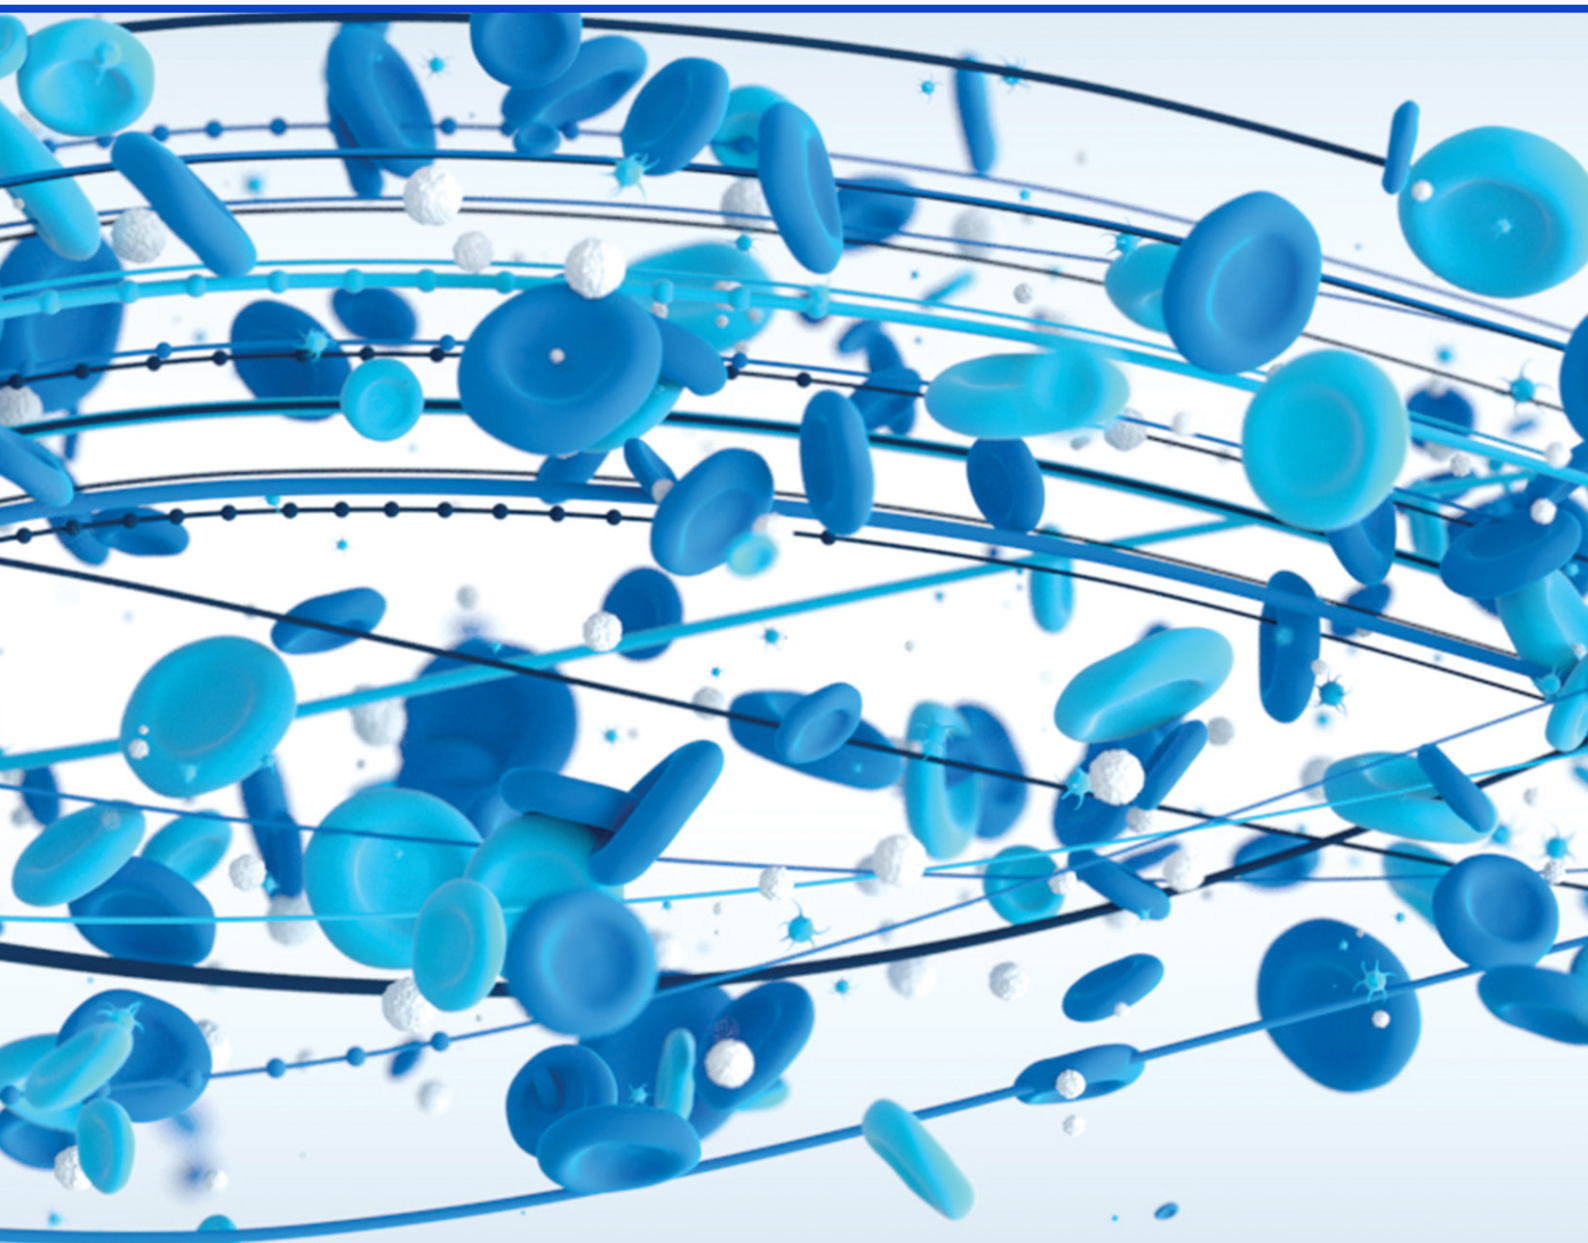

Routine and specialized testing in the Core lab

Coagulation testing is a key component of laboratory services within healthcare systems.

Coagulation tests may be requested to assess blood clotting function in a variety of clinical situations, ranging from unexplained bleeding episodes and thrombotic events, to pre-operative risk assessment.

1. Büchsel M, Creaghan J, Geisen U, Jilma P, Jones R, Kitchen S, et al. Multicentre performance evaluation and reference range for the quantitative determination of factor IX activity on the cobas t 711 analyser [abstract]. 30th Congress of the International Society on Thrombosis and Haemostasis (ISTH). 2022: PB1060. [\[link\]](#)
2. Büchsel M, Creaghan J, Geisen U, Jilma P, Jones R, Kitchen S, et al. Multicentre performance evaluation and reference range for an immunoassay for the quantitative determination of factor XIII antigen on the cobas t 711 analyser [abstract]. 30th Congress of the ISTH. 2022: PB1061. [\[link\]](#)
3. Zhu C, Sun L, Li H, Dong Z, Yu S, Zhao X, et al. Assessment and establishment of a reference interval for Roche cobas t 711 coagulation analyzer for a hospital in China. *Pract Lab Med*. 2022;29:e00268. [\[link\]](#)
4. Lowe AE, Jones R, Kitchen S, Geisen U, Rozsnyai G, Jilma P, et al. Multi-center performance evaluation and reference range determination of a new one-stage factor VIII assay. *J Clin Lab Anal*. 2022:e24294. [\[link\]](#)
5. Ketteler C, Hoffmann I, Davidson S, Tiede A, Richter N. Impact of characteristic inhibition kinetics of different FVIII inhibitors on the inhibitor titer quantification in the modified Nijmegen-Bethesda assay. *Res Pract Thromb Haemost*. 2021; 5(Suppl 2):LPB0061. [\[link\]](#)
6. Büchsel M, Creaghan J, Geisen U, Jilma P, Jones R, Kitchen S, et al. Multicenter performance evaluation and reference range determination for the quantitative assessment of factor XI activity by one-stage factor assay on the cobas t 711 analyzer. *Res Pract Thromb Haemost*. 2021;5(Suppl 2): OC451. [\[link\]](#)
7. Büchsel M, Creaghan J, Geisen U, Jilma P, Jones R, Kitchen S, et al. Multicenter performance evaluation and reference ranges for the quantitative determination of factor XII activity by one-stage factor assay on the cobas t 711 analyzer. *Res Pract Thromb Haemost*. 2021;5(Suppl 2):PB0036. [\[link\]](#)
8. Ketteler C, Hoffmann I, Davidson S, Tiede A, Richter N. Monitoring of different factor VIII replacement products using a factor VIII one-stage clotting assay on cobas t 511/711 analysers. *Haemophilia*. 2021;27(6):e704-e712. [\[link\]](#)

9. Bertsch T, Blaschke S, Body R, Davidson S, Guo G, Horner D, et al. Clinical performance of the Tina-quant D-Dimer Gen 2 assay on the cobas t 711 analyzer for evaluation of patients with suspected deep vein thrombosis (DVT) and / or pulmonary embolism (PE). *Res Pract Thromb Haemost.* 2020;4(Suppl 1):PB0600. [\[link\]](#)
10. Peyvandi F, Kenet G, Pekrul I, Pruthi RK, Ramge P, Spannagl M. Laboratory testing in hemophilia: impact of factor and non-factor replacement therapy on coagulation assays. *J Thromb Haemost.* 2020;18(6):1242-1255. [\[link\]](#)
11. Gosch I, Oberstraß J, Thelemann C. Method comparison of eight coagulation assays on the cobas t 411 versus cobas t 511/t 711 analysers. *Res Pract Thromb Haemost.* 2020;4(Suppl 1):PB0553. [\[link\]](#)
12. Ketteler C, Hoffmann I, Jagdhuber F, Davidson S, Richter N. Monitoring of different FVIII replacement drugs using the FVIII one-stage clotting assay on cobas t 511/711 analyzers. *Res Pract Thromb Haemost.* 2020;4(Suppl 1):PB0643. [\[link\]](#)
13. Geisen U, Quehenberger P, Jilma P, Lowe A, Jones R, Buechsel M, et al. Multicenter performance evaluation and reference ranges for the quantitative determination of Factors II, V, and VII by one-stage factor assay on the cobas t 711 analyzer. *Res Pract Thromb Haemost.* 2020;4(Suppl 1):PB0564. [\[link\]](#)
14. De Maat MPM, Quehenberger P, Jilma P, Kitchen S, Lowe A, Jones R, et al. Multicenter performance evaluation of the protein C chromogenic assay on the cobas t 711 analyzer. *Res Pract Thromb Haemost.* 2020;4(Suppl 1):PB0529. [\[link\]](#)
15. Jones R, Kitchen S, Geisen U, Rozsnyai G, Jilma P, Quehenberger P. Multicentre performance evaluation and reference ranges for a new assay for quantitative determination of von Willebrand factor (vWF) activity. *Res Pract Thromb Haemost.* 2020;4(Suppl 1):PB0559. [\[link\]](#)
16. Hoffmann M, Gottschalk N, Huber P, von Allmen-Zürcher N. Sample stability for a broad panel of coagulation assays on the cobas t 711 analyser using plasma stored under different conditions. *Res Pract Thromb Haemost.* 2020;4(Suppl 1): PB0545. [\[link\]](#)
17. Kitchen S, de Maat M, Nagler M, Jones R, Lowe A, Burden J, et al. System performance evaluation of the cobas t 711 and cobas t 511 coagulation analyzers in routine laboratory settings. *Blood Coagul Fibrinolysis.* 2020;31(7):459-468. [\[link\]](#)
18. Rozsnyai R, Kitchen S, Lowe A, Jones R, Geisen U, Stroobants A. Method comparison of eight new coagulation assays on the cobas t 411 analyser. *Ind J Clin Biochem.* 2019;34(Suppl 1):S157. [\[link\]](#)
19. Lippi G, Salvagno GL, Gelati M, Poli G, Giavarina D, Favaro EJ. Analytical Assessment of the New Roche Cobas t711 Fully Automated Coagulation Analyzer. *Semin Thromb Hemost.* 2019;45(03):308-314. [\[link\]](#)

20. Hoffman I, Jagdhuber F, Chen D, Davidson S, Richter N. Analytical Performance of a Modified One-stage Clotting Assay for Measuring Emicizumab on Cobas t 511/711 Analyzers. *Res Pract Thromb Haemost.* 2019;3(Suppl 1);PB1297. [\[link\]](#)
21. Jones R, Lowe A, Kitchen S, Geisen U, Stroobants A, Rozsnyai G. Analytical performance of eight new coagulation assays on the cobas t 411 analyser. *Ind J Clin Biochem.* 2019;34 (Suppl 1):S157. [\[link\]](#)
22. Lowe A, de Maat MPM, Geisen U, Jilma P, Jones R, Pfeiffer J, et al. Analytical Performance of the Factor X Assay on the cobas t 711 Analyser. *Res Pract Thromb Haemost.* 2019;3(Suppl 1);PB0118. [\[link\]](#)
23. Quehenberger P, Jilma P, Jones R, Kitchen S, Lowe A, Rozsnyai G, et al. Analytical performance of the free protein S assay on the cobas t 711 analyser. *Res Pract Thromb Haemost.* 2019;3(Suppl 1); PB0108. [\[link\]](#)
24. Geisen U, Jilma P, Jones R, Kitchen S, Lowe A, Pfeiffer J, et al. Analytical performance of the Lupus screen and Lupus confirm assays on the cobas t 711 analyser. *Res Pract Thromb Haemost.* 2019;3(Suppl 1);PB0116. [\[link\]](#)
25. Salvagno GL, Lippi G, Gelati M, Poli G, Favaro E. Analytical performance of the new D-dimer and antithrombin assay on Roche cobas t 711 analyzer. *Int J Lab Hematol.* 2019;41(3):e54-e56. [\[link\]](#)
26. Oostendorp M, Noorman RL, Nijenhuis JD, de Kok JB. Performance of 6 routine coagulation assays on the new Roche cobas t711 analyzer. *Pract Lab Med.* 2019;17:e00146. [\[link\]](#)
27. Kappelmayer J, Mázló A, Kerényi A. Evaluation of the analytical performance of von Willebrand factor antigen and activity tests on the Cobas t 511 coagulation analyser. *Hamostaseologie.* 2019;39(S01):P10-5. [\[link\]](#)
28. Kitchen S, Geisen U, Kappelmayer J, Quehenberger P, Drieß J, Lowe A, et al. Evaluating the analytical performance of five new coagulation assays for the measurement of prothrombin time and activated thromboplastin time. *Int J Lab Hematol.* 2018;40(6):645-654. [\[link\]](#)
29. Kitchen S, Geisen U, Kappelmayer J, Quehenberger P, Lowe A, Jones R, et al. Evaluating the analytical performance of four new coagulation assays for the measurement of fibrinogen, D-dimer and thrombin time. *Int J Lab Hematol.* 2018;40(6):637-644. [\[link\]](#)
30. Lippi G, Favaro E. Laboratory hemostasis: from biology to the bench. *Clin Chem Lab Med.* 2018;56(7):1035-1045. [\[link\]](#)
31. Geisen U, Kappelmayer J, Jones R, Lowe A, Miles G, Rozsnyai G, et al. Method comparison of the PT Rec coagulation assay with existing reference methodology for measuring prothrombin time (PT). *Res Pract Thromb Haemost.* 2018;2(Suppl 1):PB0246. [\[link\]](#)

32. Quehenberger P, Geisen U, Kappelmayer J, Jones R, Lowe A, Miles G, et al. Precision and method comparison data for three new coagulation assays measuring activated partial thromboplastin time (aPTT) on the new cobas t 711 and t 511 analysers. 70th AACC Annual Scientific Meeting Abstracts. 2018:A311. [\[link\]](#)
33. Geisen U, Drieß J, Burden J, Rozsnyai G, Wu J, Kitchen S. Sensitivity of the aPTT, aPTT Lupus and aPTT Screen assays towards heparin and lupus anticoagulant. 70th AACC Annual Scientific Meeting Abstracts. 2018:A313. [\[link\]](#)
34. Lowe A, Kitchen S, Jones R, de Maat MPM, Nagler M, Rozsnyai G. System performance evaluation of the cobas t 711 and cobas t 511 analysers. *Res Pract Thromb Haemost.* 2018;2(Suppl 1):PB256. [\[link\]](#)
35. Kitchen S, Geisen U, Kappelmayer J, Quehenberger P, Jones R, Lowe A, et al. Evaluating the analytical performance of six new coagulation assays. *Res Pract Thromb Haemost.* 2017;1 (Supp 1):PB0428. [\[link\]](#)
36. Lowe A, Kitchen S, Adcock D, Gegen R, Crawford M, Grant R, et al. Impact of Rivaroxaban and Dabigatran on clotting screens as performed using the Roche cobas t 711 analyser. *Res Pract Thromb Haemost.* 2017;1(Supp 1):PB1157. [\[link\]](#)



Coagulation bedside testing

Coagulation Point-of-Care Testing (POCT or bedside testing) allows for medical diagnostic testing at the time and place of patient care, enabling physicians to quickly and reliably diagnose conditions and adjust hemostatic therapy.

Patient self-testing (PST) and patient self-management (PSM) allow convenient testing and dosage adjustment of vitamin K antagonists (VKAs) to maintain a high time in therapeutic range (TTR), which is linked to a reduction in adverse events.

1. Pulcer M, Gumulec J, Recova L, Kolarova S, Svagera Z, Stejskal D. The Comparison of Critical Care Instrument CoaguChek® Pro II with Coagulation Analyzers Sysmex CS-5100 and Cobas t 511. *Res Pract Thromb Haemost.* 2020;4(Suppl 1):PB0284. [\[link\]](#)
2. Arachchilage DR, Vipond L, Laffan M. Limitations on point care APTT for monitoring of unfractionated heparin in intensive care patients. *Thromb Res.* 2019;181:124-126. [\[link\]](#)
3. Baker WS, Albright KJ, Berman M, Spratt H, Mann PA, Unabia J, et al. POCT PT INR – Is it adequate for patient care? A comparison of the Roche CoaguChek XS vs. Stago Star vs. Siemens BCS in patients routinely seen in an anticoagulation clinic. *Clin Chim Acta.* 2017;472:139-145. [\[link\]](#)
4. Plesch W, van den Besselaar AMHP. Validation of the international normalized ratio (INR) in a new point-of-care system designed for home monitoring of oral anticoagulation therapy. *Int J Lab Hematol.* 2009;31(1):20-25. [\[link\]](#)
5. Wieloch M, Hillarp A, Strandberg K, Nillson C, Svensson PJ. Comparison and evaluation of a Point-of-care device (CoaguChek XS) to Owren-type prothrombin time assay for monitoring of oral anticoagulant therapy with warfarin. *Thromb Res.* 2009;124(3):344-348. [\[link\]](#)
6. Ryan F, Byrne S, O'Shea S. Randomized controlled trial of supervised patient self-testing of warfarin therapy using an internet-based expert system. *J Thromb Haemost.* 2009;7(8):1284-1290. [\[link\]](#)
7. Plesch W, Wolf T, Breitenbeck N, Dikkenschei LD, Cervero A, Perez PL, et al. Results of the performance verification of the CoaguChek XS system. *Thromb Res.* 2008;123(2):381-389. [\[link\]](#)
8. Gardiner C, Williams K, Mackie IJ, Machin SJ, Cohen H. Patient self-testing is a reliable and acceptable alternative to laboratory INR monitoring. *Br J Haematol.* 2005;128(2):242-247. [\[link\]](#)



Platelet aggregometry

Platelets play a vital role in normal haemostasis, with inherited or acquired dysfunctions involved in an array of bleeding disorders and thrombotic events. Platelet aggregometry testing is applied in a variety of clinical situations, e.g, in monitoring response to antiplatelet therapy, assessment of perioperative bleeding risk and detection of platelet dysfunction in POCT and routine settings.

1. Sibbing D, Aradi D, Alexopoulos D, Ten Berg J, Bhatt DL, Bonello L, et al. Updated Expert Consensus Statement on Platelet Function and Genetic Testing for Guiding P2Y(12) Receptor Inhibitor Treatment in Percutaneous Coronary Intervention. *JACC Cardiovasc Interv.* 2019;12(16):1521-1537. [\[link\]](#)
2. Sibbing D, Aradi D, Jacobshagen C, Gross L, Trenk D, Geisler T, et al. Guided de-escalation of antiplatelet treatment in patients with acute coronary syndrome undergoing percutaneous coronary intervention (TROPICAL-ACS): a randomised, open-label, multicentre trial. *Lancet.* 2017;390(10104):1747-1757. [\[link\]](#)
3. Kong R, Trimmings A, Hutchinson N, Gill R, Agarwal S, Davidson S, et al. Consensus recommendations for using the Multiplate(®) for platelet function monitoring before cardiac surgery. *Int J Lab Hematol.* 2015;37(2):143-147. [\[link\]](#)
4. Galea V, Khaterchi A, Robert F, Gerotziafas G, Hatmi M, Elalamy I. Heparin-induced multiple electrode aggregometry is a promising and useful functional tool for heparin-induced thrombocytopenia diagnosis: confirmation in a prospective study. *Platelets.* 2013;24(6):441-447. [\[link\]](#)



COBAS is a trademark of Roche.

© 2022 Roche

Published by:

Roche Diagnostics International Ltd
CH-6343 Rotkreuz
Switzerland

diagnostics.roche.com