

Ordering information

Product	Material configuration	Material number
Elecsys® SARS-CoV-2 Antigen ^{a)}	200 tests	09 345 272 190
Elecsys® SARS-CoV-2 Antigen ^{b)}	300 tests	09 345 299 190
PreciControl SARS-CoV-2 Antigen	6 × 2.0 mL	09 345 302 190
SARS-CoV-2 Extraction Solution	1,000 mL	09 370 064 190
SARS-CoV-2 Extraction Solution C	500 mL	09 370 099 190

a) for use on the **cobas e** 411 analyzer and the **cobas e** 601 / 602 modules; b) for use on the **cobas e** 801 module

Elecsys® SARS-CoV-2 Antigen

Immunoassay for the qualitative detection of the SARS-CoV-2 nucleocapsid antigen

Summary

SARS-CoV-2, the causative agent of COVID-19, is an enveloped, single-stranded RNA Betacoronavirus.¹⁻³ 7 coronaviruses have been identified as agents of human infection, causing disease ranging from mild common cold to severe respiratory failure.⁴ Coronaviruses share the 4 structural proteins spike (S), envelope (E), membrane (M), and nucleocapsid (N), the latter being the most abundant.⁵⁻⁸


SARS-CoV-2 is transmitted primarily from person-to-person through respiratory droplets and aerosols.^{9,10} The incubation period from infection to detectable viral load in the host commonly ranges from 2 to 14 days.^{11,12} Detection of viral load can be associated with the onset of clinical signs and symptoms, although a considerable proportion of individuals remains asymptomatic or mildly symptomatic.¹³⁻¹⁵ The interval during which an individual with COVID-19 is infectious has not yet been clearly established, however, transmission from symptomatic, asymptomatic, and pre-symptomatic individuals has been well described.¹⁶⁻¹⁸

An effective strategy for controlling the COVID-19 pandemic is to develop highly accurate methods for the identification and isolation of SARS-CoV-2 infected patients.¹⁹ Diagnostic confirmation of acute SARS-CoV-2 infection can be based on the detection of unique sequences in the viral RNA or

detection of viral proteins in respiratory tract samples from infected individuals.²⁰ Viral antigens are only expressed when the virus is actively replicating, thus making antigen tests clinically useful for identification of acute or early infection.^{21,22} Current research suggests active replication of SARS-CoV-2 in the throat with high viral shedding in the first 5 days of infection, and infectious virus could be isolated from respiratory samples up to the first 7–9 days post symptom onset, indicating potential feasibility of antigen detection using throat swabs.²³⁻²⁵ This time period also coincides with the time when the highest viral load is generally observed in infected individuals.^{14,26-28} Therefore, the best performance of antigen tests is seen around symptom onset in symptomatic individuals and the initial phase of infection.²⁰ Testing of mildly symptomatic or asymptomatic individuals can be considered in the assessment of contacts of confirmed infected persons.²⁰ Antigen tests can also become part of regular testing regimens for identifying, isolating, and thus filtering out currently infected persons, including those who are asymptomatic.^{29,30}

The Elecsys® SARS-CoV-2 Antigen assay uses monoclonal antibodies directed against the SARS-CoV-2 N protein in a double-antibody sandwich assay format for the qualitative detection of SARS-CoV-2 in upper respiratory tract specimens.³¹

Structure of the Severe Acute Respiratory Syndrome Coronavirus 2 (SARS-CoV-2)

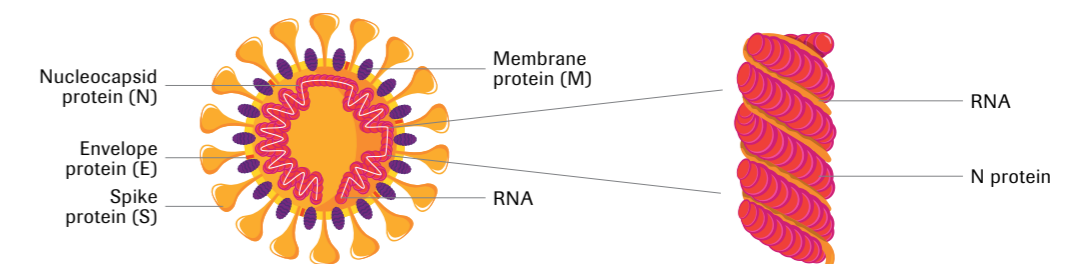

References

- Zhou, P. et al. (2020). *Nature* 579(7798), 270-273.
- Wu, F. et al. (2020). *Nature* 579(7798), 265-269.
- Coronaviridae Study Group of the International Committee on Taxonomy of Viruses (2020). *Nat Microbiol.* 5(4), 536-544.
- Ye, Z.W. et al. (2020). *Int J Biol Sci.* 16(10), 1686-1697.
- Yoshimoto, F.K. (2020). *Protein J* 39(3), 198-216.
- Naqvi, A.A.T. et al. (2020). *Biochim Biophys Acta Mol Basis Dis.* 1866(10), 165878.
- Ke, Z. et al. (2020). *Nature.* doi:10.1038/s41586-020-2665-2.
- Bezstarosti, K. et al. (2020). *bioRxiv* 2020.04.23.057810.
- Zhu, N. et al. (2020). *N Engl J Med.* 382(8), 727-733.
- World Health Organization (2020). Available from: <https://www.who.int/news-room/commentaries/detail/transmission-of-sars-cov-2-implications-for-infection-prevention-precautions>.
- Chan, J.F. et al. (2020). *Lancet* 395(10223), 514-523.
- Lauer, S.A. et al. (2020). *Ann Intern Med.* 72(9), 577-582.
- Zhou, R. et al. (2020). *Int J Infect Dis.* 96, 288-290.
- He, X. et al. (2020). *Nature Medicine.* 26(5), 672-675.
- Mizumoto, K. et al. (2020). *Euro Surveill.* 25(10), pii=2000180.
- Gao, M. et al. (2020). *Respir Med.* 169, 106026.
- Yu, P. et al. (2020). *J Infect Dis.* 221(11), 1757-1761.
- Liu, Z. et al. (2020). *Int J Infect Dis.* 99, 325-327.
- Ji, T. et al. (2020). *Biosens Bioelectron.* 166, 112455.
- World Health Organization (2020). Available at: <https://www.who.int/publications-detail-redirect/diagnostic-testing-for-sars-cov-2>.
- World Health Organization (2020). Available at: <https://www.who.int/newsroom/commentaries/detail/advice-on-the-use-of-point-of-care-immunodiagnostic-tests-for-covid-19>.
- Centers for Disease Control and Prevention (2020). Available at: <https://www.cdc.gov/coronavirus/2019-ncov/lab/resources/antigen-tests-guidelines.html>.
- Bullard, J. et al. (2020). *Clin Inf Dis.* ciaa638, doi:10.1093/cid/ciaa638.
- Woelfel, R. et al. (2020). *Nature* 581(7809), 465-469.
- World Health Organization (2020). Available at: <https://apps.who.int/iris/handle/10665/332451>.
- Weiss, A. et al. (2020). *EBioMedicine* 58, 102916.
- Sethuraman, N. et al. (2020). *JAMA* 323(22), 2249-2251.
- Zou, L. et al. (2020). *N Engl J Med.* 382(12), 1177-1179.
- Larremore, D.B. et al. (2020). *medRxiv* 2020.06.22.20136309.
- Mina, M.J. et al. (2020). *N Engl J Med.* doi:10.1056/NEJMp2025631.
- Elecsys® SARS-CoV-2 Antigen. Method sheet v1 (Dec 2020).
- cobas® SARS-CoV-2, Qualitative assay for use on the cobas® 6800/8800 Systems. Method sheet, v3 (May 2020).

COBAS, COBAS E, ELECSYS and PRECICONTROL are trademarks of Roche.

All other trademarks are the property of their respective owners.


© 2020 Roche

Published by:
Roche Diagnostics International Ltd
CH-6343 Rotkreuz
Switzerland

diagnostics.roche.com

Electro-chemiluminescence immunoassay (ECLIA)

Test principle: double-antibody sandwich assay (testing time: 18 minutes)³¹

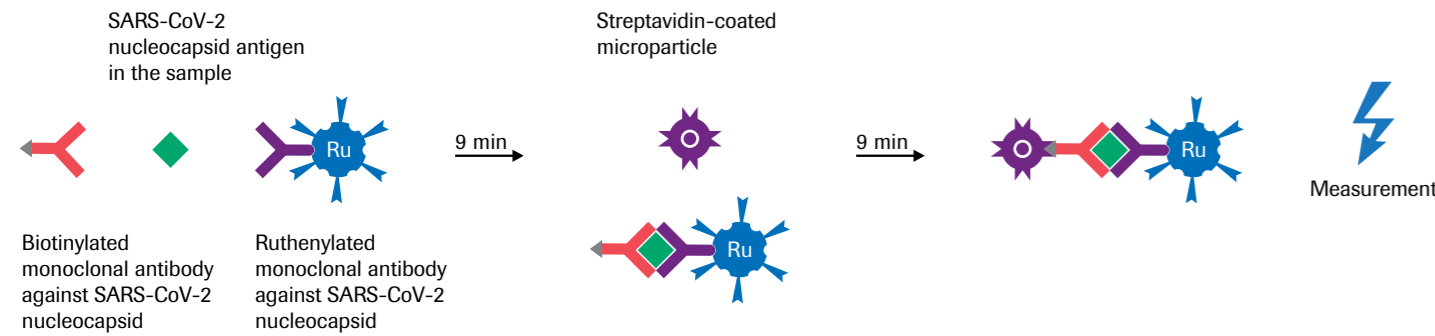

Step 1 (9 minutes)

50 µL* / 30 µL** of the patient sample are incubated with a mix of biotinylated and ruthenylated monoclonal antibodies to the SARS-CoV-2 antigen. Double-antibody sandwich (DABS) immune complexes are formed in the presence of corresponding antigen.

* **cobas e 411** analyzer and **cobas e 601/602** modules
** **cobas e 801** module

Step 2 (9 minutes)

After addition of streptavidin-coated microparticles, the DABS complexes bind to the solid phase via interaction of biotin and streptavidin.

Step 3 (measurement)

The reagent mixture is transferred to the measuring cell, where the microparticles are magnetically captured onto the surface of the electrode. Unbound substances are subsequently removed. Electrochemiluminescence is then induced by applying a voltage and measured with a photomultiplier. The signal yield increases with the antibody titer.

Elecsys® SARS-CoV-2 Antigen assay characteristics³¹

Systems	cobas e 411 analyzer cobas e 601 / cobas e 602 modules	cobas e 801 module
Testing time	18 minutes	
Test principle	One-step double antibody sandwich assay	
Calibration	2-point	
Interpretation	COI <1.0 = non-reactive, COI ≥1 = reactive	
Specimen types	Naso-/Oropharyngeal specimens, collected using flocked or polyester-tipped swabs, placed in 3 mL Copan Universal Transport Medium (UTM-RT™), BD™ Universal Viral Transport (UVT), Viral Transport Media (VTM)*, or sterile saline (0.9% NaCl)	
Sample volume	50 µL	30 µL
Onboard stability	14 days	
Intermediate** precision in positive samples	cobas e 411 analyzer: CV* 2.2 – 5.8% cobas e 601 / 602 modules: CV 1.9 – 3.5%	CV 1.7 – 5.7%

*prepared according to CDC SOP DSR-052-05; **between runs; *coefficient of variation

Limit of Detection (LoD)³¹

The limit of detection (LoD) in different transport media was determined by limiting dilution studies using an inactivated viral lysate (USA-WA1/2020). LoD is defined as the lowest detectable concentration of SARS-CoV-2 at which a minimum of 19 from 20 replicates per concentration generate a reactive test result (≥1.0 COI), and expressed as TCID₅₀/mL.

Transport Medium

Transport Medium	TCID ₅₀ /mL
COPAN Universal Transport Medium (UTM-RT)	22.5
CDC Viral Transport Medium	22.5
Sterile Saline (0.9% NaCl)	37.5


*Median Tissue Culture Infectious Dose

Relative sensitivity³¹

Relative sensitivity was evaluated using 232 nasopharyngeal and 158 oropharyngeal swab specimens, collected from individuals with signs and symptoms suggestive of COVID-19, with known or suspected exposure to SARS-CoV-2, and from individuals undergoing pre-admission screening before hospitalization for surgical intervention unrelated to an infectious disease. All subjects included in the analysis were tested positive in the **cobas®** SARS-CoV-2 RT-PCR test³². RT-PCR-positive samples were further

stratified using Target 2 (structural protein envelope E-gene/pan-Sarbecovirus detection) cycle threshold (C_t) values.

The figure below correlates the performance of the Elecsys® SARS-CoV-2 Antigen assay in all RT-PCR-positive samples from symptomatic and asymptomatic individuals to the **cobas®** SARS-CoV-2 C_t values.

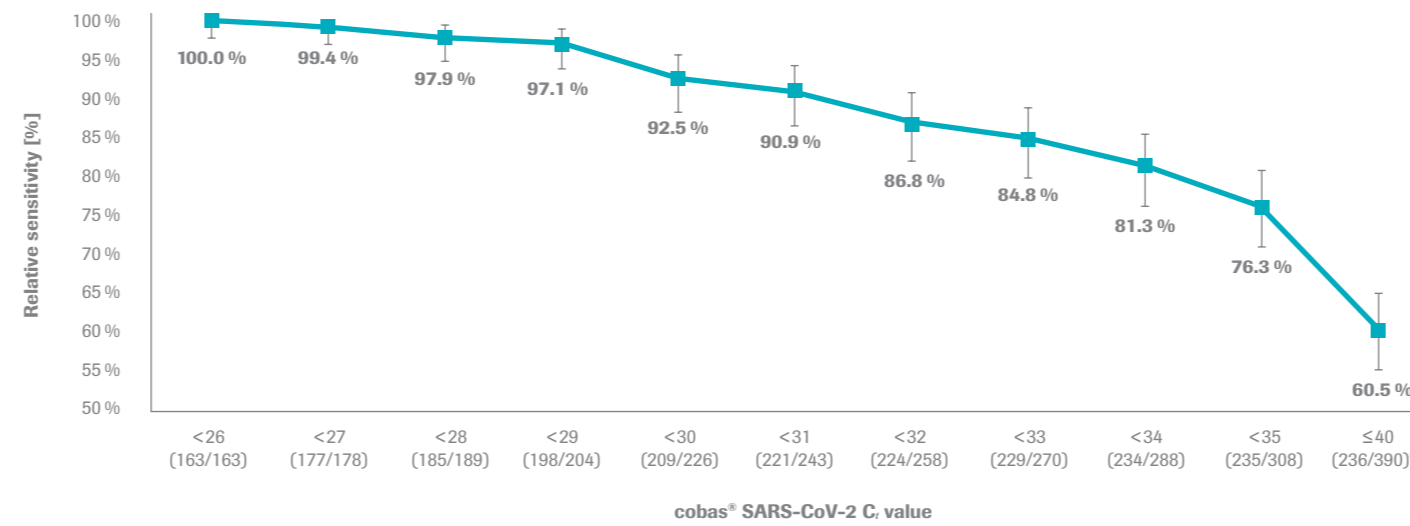


*structural protein envelope E-gene/pan-Sarbecovirus detection; **N (cumulative): reactive in the Elecsys® SARS-CoV-2 Antigen assay/total

The table below shows additional analyses based on days post-symptom onset (DPSO) and stratification by a **cobas®** SARS-CoV-2 C_t value of 30. The resulting overall relative sensitivity in symptomatic individuals with a **cobas®** SARS-CoV-2 Target 2 C_t value <30 was 94.5% (95% CI two-sided: 90.4 – 97.2% [189/200]).

Cohort	cobas® SARS-CoV-2 C _t <30			cobas® SARS-CoV-2 C _t ≥30		
	N	Non-reactive	Sensitivity (95% CI) [†]	N	Non-reactive	Sensitivity (95% CI) [†]
Symptomatic; ≤5 DPSO	119	3	97.5 % (92.8 – 99.5 %)	30	22	26.7 % (12.3 – 45.9 %)
Symptomatic; ≤10 DPSO	158	8	94.9 % (90.3 – 97.8 %)	78	60	23.1 % (14.3 – 34.0 %)
Symptomatic; >10 DPSO	4	1	75.0 % (19.4 – 99.4 %)	18	15	16.7 % (3.6 – 41.4 %)
Symptomatic; unknown DPSO	38	2	94.7 % (82.3 – 99.4 %)	17	13	23.5 % (6.8 – 49.9 %)
Known or suspected exposure	14	3	78.6 % (49.2 – 95.3 %)	34	33	2.9 % (0.1 – 15.3 %)
Screening	12	3	75.0 % (42.8 – 94.5 %)	17	16	5.9 % (0.2 – 28.7 %)

The following table summarizes the relative sensitivity of the Elecsys® SARS-CoV-2 Antigen assay in RT-PCR-positive samples from symptomatic patients, stratified by days post symptom onset, and a **cobas®** SARS-CoV-2 Target 2 C_t value of 30.

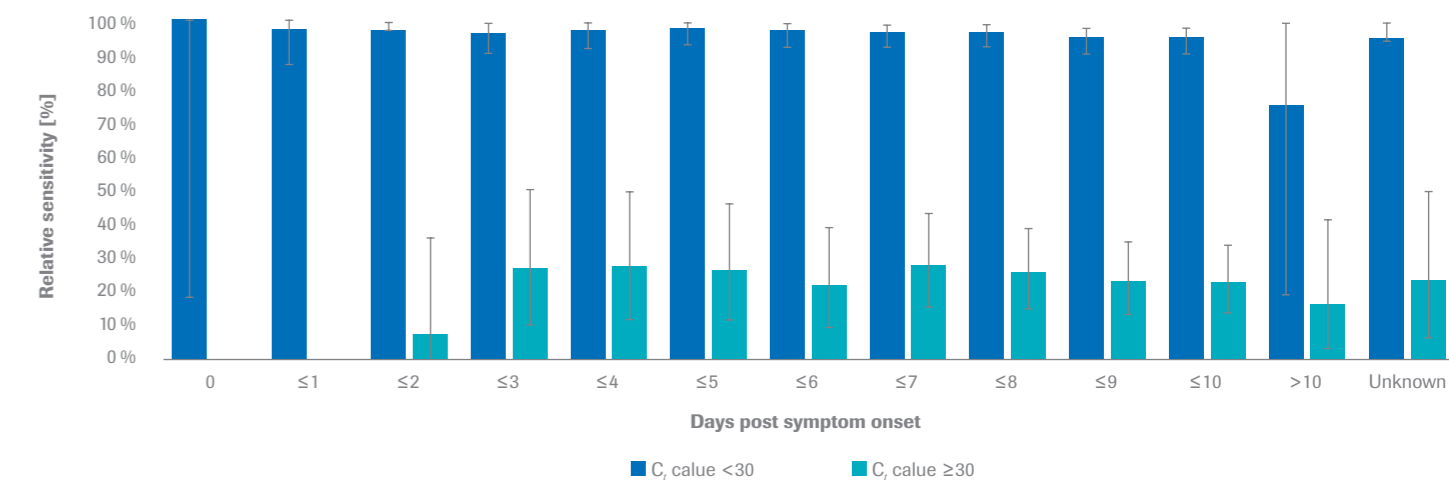

Relative specificity³¹

Relative specificity of the Elecsys® SARS-CoV-2 Antigen assay was evaluated using 2,747 RT-PCR negative naso-/oropharyngeal swab specimens, collected from individuals with signs and symptoms suggestive of COVID-19, with known or suspected exposure to SARS-CoV-2, and from individuals undergoing pre-admission screening before hospitalization for surgical intervention unrelated to an infectious disease.

Cohort	N	Reactive	Specificity (95% CI)
Symptomatic	548*	0	100 % (99.3 – 100 %)
Known/suspected exposure and screening	2,199**	4	99.8 % (99.5 – 100 %)
Overall	2,747	4	99.9 % (99.6 – 100 %)

*3; **12 samples invalid with **cobas®** SARS-CoV-2 RT-PCR, but negative with another SARS-CoV-2 RT-PCR test

Estimated course of markers in SARS-CoV-2 infection^{27,30}

