

---

To:                   Stefan Grigarczik                   Copies:  
                          Kornelius Wiechmann               Bernard Scheffler  
                          Corinna Baust                        Ingrid Leichsenring  
  Petra Herbel

---

From:                Johannes Hayer                   DXRDDD  
  Building / Room 272 R 602  
  Phone: +49-621 759 5248  
  Mail: Johannes.hayer@roche.com

---

Date:                08. August 2016

---

## **Memo\_aPTT\_T\_0101, Version 2.0**


### **Traceability for blood measurements of the CoaguChek aPTT Test on the CoaguChek Pro II System**

#### **1. Intention**

A concept for traceability for blood measurements is developed for the CoaguChek aPTT Test on the CoaguChek Pro II System.

## 2. Traceability Chain

The traceability chain for the CoaguChek aPTT Test (CC aPTT Test) can be displayed as follows:

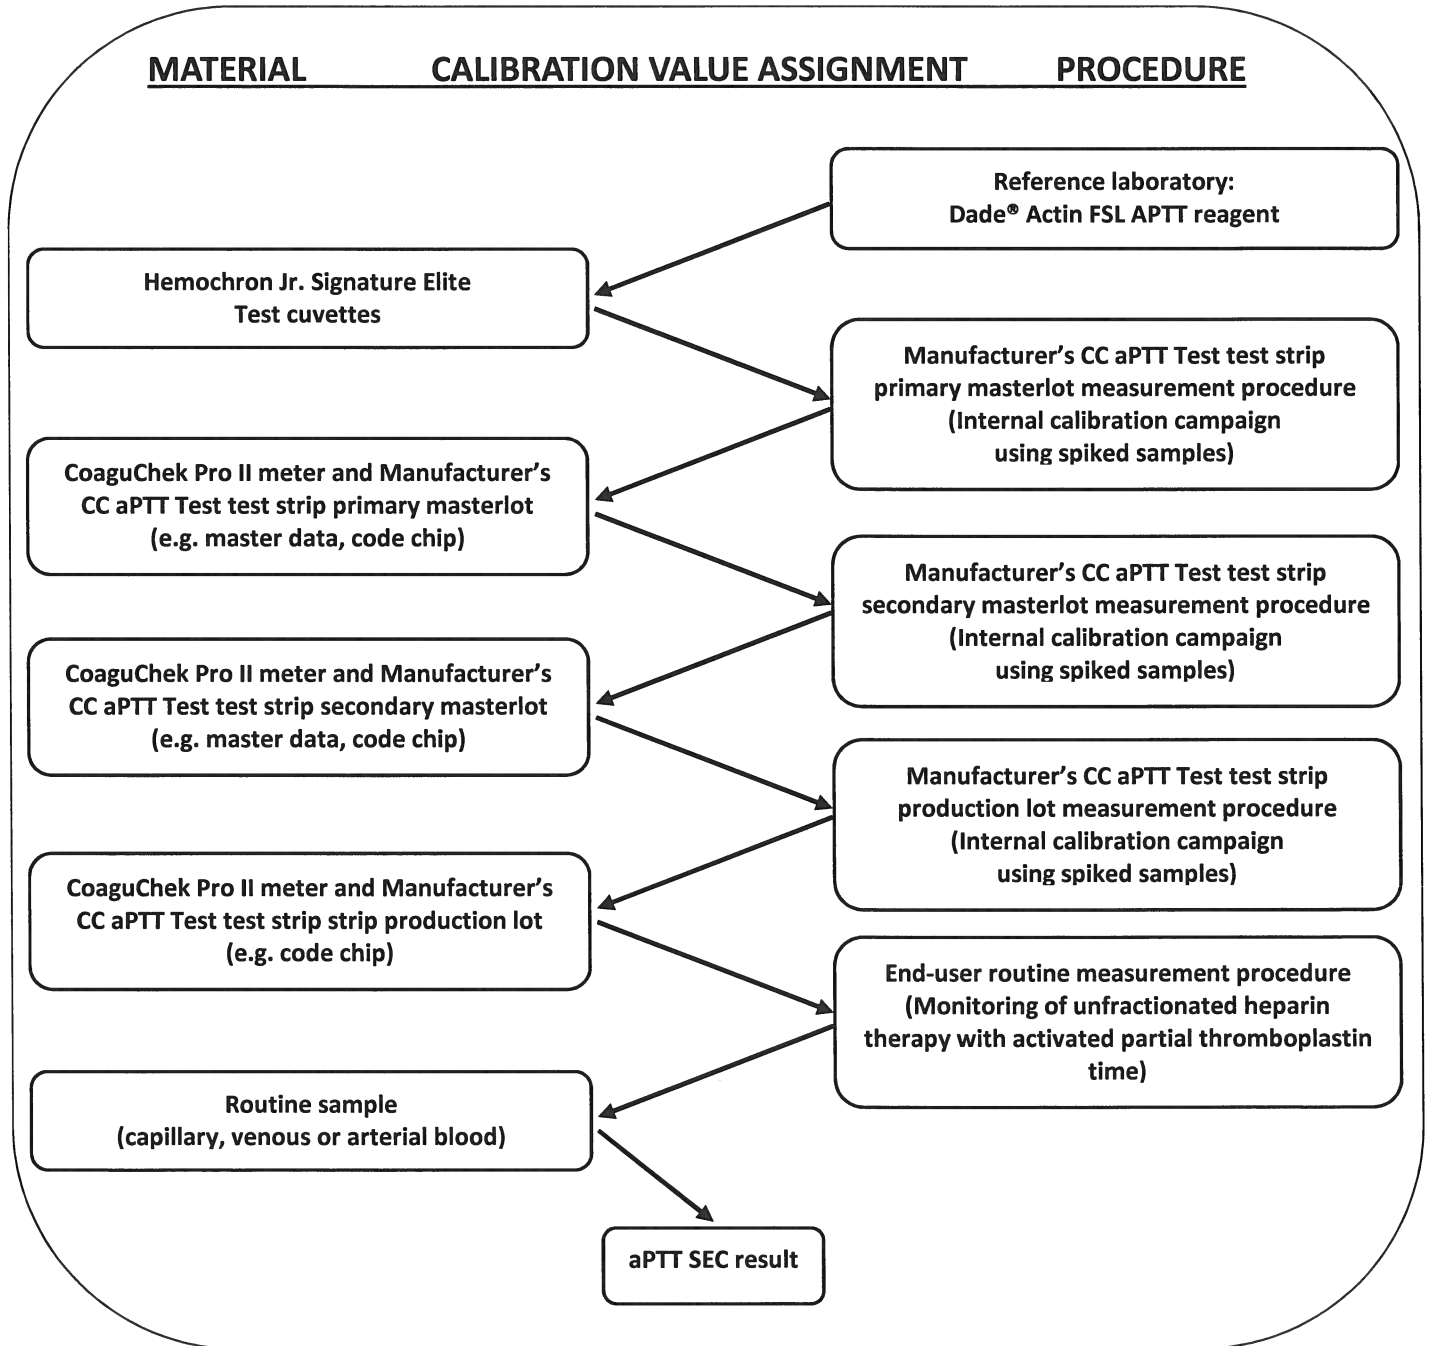

**Figure:** Traceability chain for a measurement result of the oral anticoagulation monitoring system CoaguChek Pro II with the CoaguChek aPTT Test to the reference method

08-Aug-2016 *J. Hayer*  
 Author: J. Hayer, DXRDDD

08-Aug-2016 *I. Leichsenring*  
 Reviewer: I. Leichsenring, DXRDDD